


Circuits consumption in 7 days waste

28 patients

Ø 4 patients / 24 h

Single use

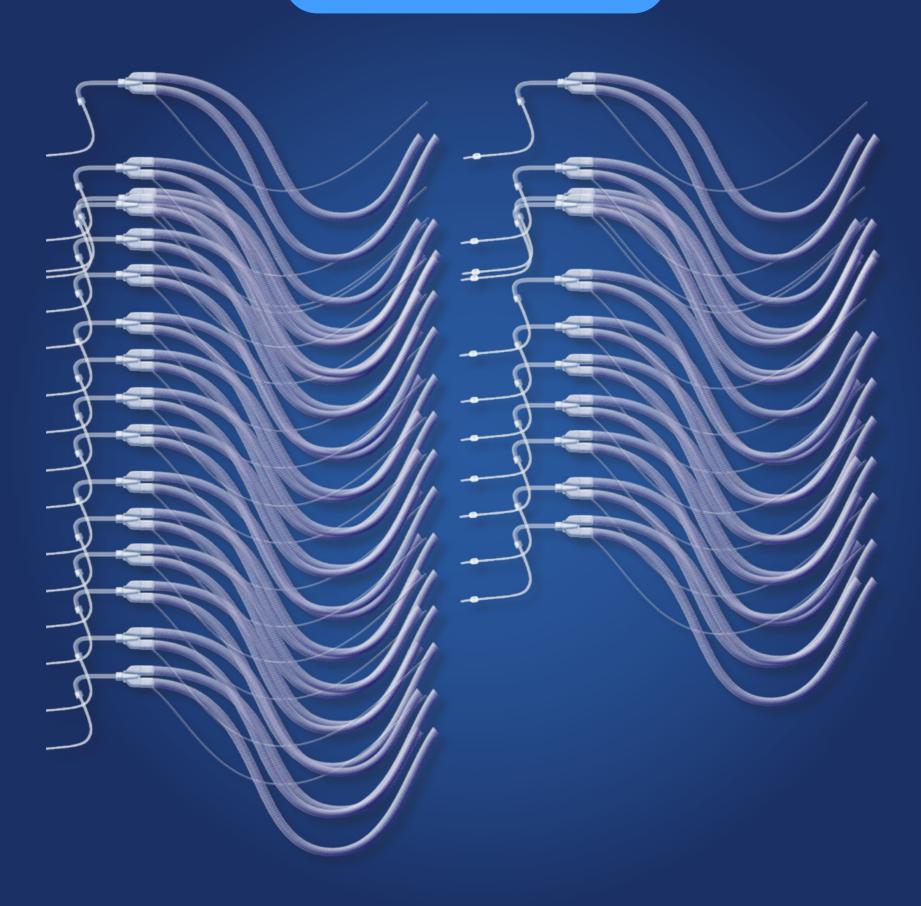

Change after 24 hours (once a day)

